

SMALL SCALE REACTION CALORIMETRY

A. Zogg*, U. Fischer**, K. Hungerbühler**

*andreas.zogg@cibasc.com, Ciba Specialty Chemicals, Schweizerhalle, Basel.

**ulrich.fischer@tech.chem.ethz.ch, Safety and Environmental Technology Group, Laboratory of Technical Chemistry, Institute for Chemical and Bioengineering, Swiss Federal Institute of Technology (ETH), ETH Hönggerberg, HCI G133, CH-8093 Zurich, Switzerland

To meet the need for a systematic and quick gathering of **kinetic and thermodynamic reaction parameters** in early phases of process design a **small reaction calorimeter (25 to 45 ml) with an integrated IR-ATR probe** was developed during this work.^{1,2,6} The new prototype reaction calorimeter (see Fig.1) uses a copper block as an intermediate thermostat instead of a double wall vessel (typically glass) with a circulation fluid.

The reaction temperature is controlled at **isothermal conditions using the Power-Compensation principle**. To allow an **online measured baseline** (compensate changes of the heat transfer through the reactor wall during the reaction) **an additional heat-flow balance using Peltier elements is implemented and was patented**.¹ Due to this combination **no calibration steps are**

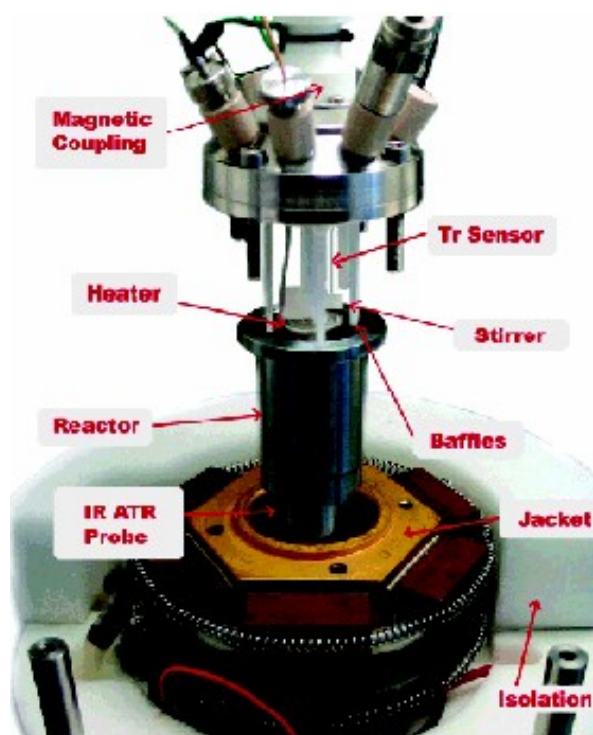


Fig. 1 Latest version of the small-scale reaction calorimeter (sample volume 20 - 45 ml) with reactor jacketed made of copper and removable reactor (Hasteloy C22). The reactor is pressure resistant up to 20 bar, Temperature rage -20 ... 200 °C.⁶

required, and several devices could be connected to the same cryostat (parallelisation). The new calorimeter has a very **small time constant of about 4 s** (time constant of the jacket about 15 s) and is therefore ideally suited to measure **fast and highly exothermal** reactions at isothermal conditions.^{2,5,6}

The performance and the accuracy of the new device will be demonstrated based on several reaction examples: The **neutralization of NaOH with H₂SO₄**, the **hydrolysis of acetic anhydride**, as well as two **highly exothermal industrial reactions** (maximal reaction power of ≈ 2.5 kW/l).

Furthermore a **new evaluation principle** for the measured reaction was developed^{2,3,4,5} that allows the identification of the unknown reaction parameters such as rate constants, activation energies, reaction orders and reaction enthalpies. The evaluation is based on an empirical reaction model. **In contrast to conventional evaluation procedures the infrared and calorimetric data are simultaneously evaluated**. Only a short introduction into this evaluation algorithm will be given.

References

- (1) A. Zogg, M. Wohlwend, U. Fischer, K. Hungerbühler, **2000**, EP 1184649.
- (2) Zogg, A., **2003**, Dissertation ETH Nr. 15086.
- (3) Zogg, A., U. Fischer, and K. Hungerbühler, **2004**, Chemical Engineering Science 59(24), 5795-5806.
- (4) Zogg, A., U. Fischer, and K. Hungerbühler, **2004**, Chemometrics and Intelligent Laboratory Systems 71: 165-176.
- (5) Zogg, A., F. Stoessel, U. Fischer, and K. Hungerbühler, **2004**, Thermochemica Acta, 419: 1-17.
- (6) Visentin, F., S.I. Gianoli, A. Zogg, O.M. Kut, and K. Hungerbühler, **2004**, Organic Process Research & Development 8: 725-737.